smiths medical portex

EzPAP[®] Positive Airway Pressure Therapy System Set-Up Guidelines

SET FLOW RATE

Begin at 5 LPM [fig 2]. Increase until desired PAP is reached. (Do not exceed 15 LPM.)

2 VERIFY PRESSURE

Should not exceed 20cm H₂0 [fig 1].

BREATHE

Patient should be instructed to inhale and exhale slowly [fig 3].




NOTE: Refer to individual product Instructions For Use for warnings, cautions, contraindications, and additional information

Smiths Medical International Ltd Hythe, Kent CT21 6JL, UK Tel: (0)1303 260551 www.smiths-medical.com Smiths Medical ASD Inc 1500 Eureka Park, Lower Pemberton Ashford Kent, TN25 4BF Tel: +44 (0)845 850 0445



Caution: Federal law (USA) restricts this device to sale by or on the order of a physician. EzPAP® and Smiths Medical design mark are trademarks of the Smiths Medical. The symbol ® indicates the trademark is registered in the U.S. Patent and Trademark Office and certain other countries. © 2016 Smiths Medical. All rights reserved. RE194235GB-102016

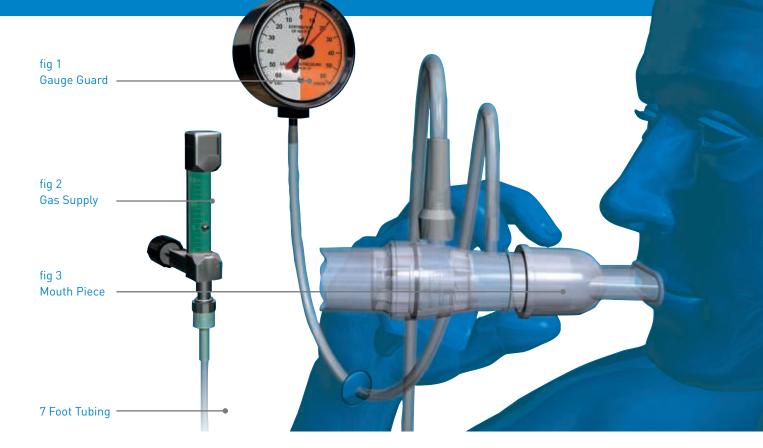

smiths medical